

NBSIR 77-855

FILE COPY
DO NOT REMOVE

QUARTZ CRYSTAL OSCILLATORS WITH LOW ACCELERATION SENSITIVITY

RECEIVED
DATE 4/7/77
OTP

J. J. Gagnepain
F. L. Walls

Time and Frequency Division
Institute for Basic Standards
National Bureau of Standards
Boulder, Colorado 80302

March 1977

NBSIR 77-855

QUARTZ CRYSTAL OSCILLATORS WITH LOW ACCELERATION SENSITIVITY

J. J. Gagnepain
F. L. Walls

Time and Frequency Division
Institute for Basic Standards
National Bureau of Standards
Boulder, Colorado 80302

March 1977



U.S. DEPARTMENT OF COMMERCE, Juanita M. Kreps, Secretary

Dr. Betsy Ancker-Johnson, Assistant Secretary for Science and Technology

NATIONAL BUREAU OF STANDARDS, Ernest Ambler, Acting Director

J. J. Gagnepain* and F. L. Walls**

The acceleration sensitivity of quartz crystal resonators imposes severe limitation on their use in non-laboratory environments. This work shows that by using two resonators connected in series and properly orientated with respect to one another, it is possible to substantially reduce the net acceleration sensitivity of the composite or compound crystal resonator. First qualitative experimental results on acceleration, also some experimental theories of studies related to the introduction of the two resonators comprising the compound resonator, are presented. From these studies it appears feasible to fabricate compound crystal resonators exhibiting acceleration sensitivities at least 10 times smaller than the resonators used individually.

Key words: Acceleration field; acceleration sensitivity; compound crystal resonator; crystallographic axis; non-linear elastic effect; resonance frequency.

When a quartz crystal resonator is in an acceleration field, the induced body forces and the reaction forces give a static or quasistatic deformation. Because of the non-linear elastic effects, an interaction occurs between the elastic wave and this static deformation, changing the wave velocity, and by a small amount, the crystal sizes. The result is a variation of the resonance frequency, related to the applied acceleration field direction, as shown in Fig. 1 [1].

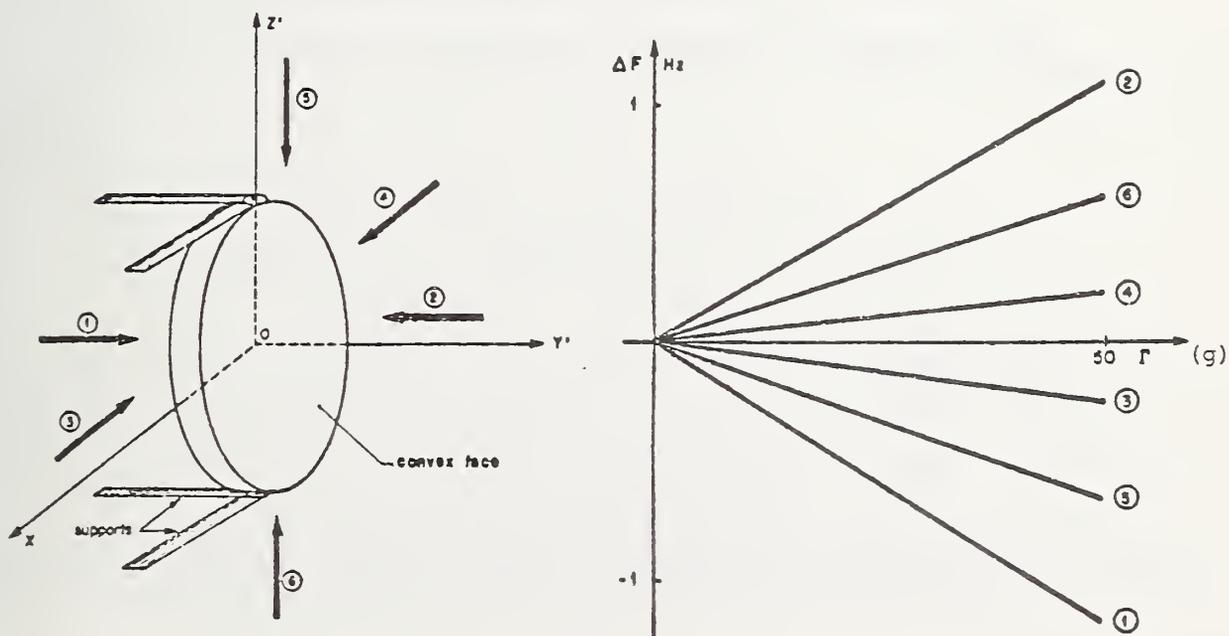


FIGURE 1 Frequency variation of a quartz resonator for several different directions of applied force.

* Laboratoire de Physique et Metrologie des Oscillateurs

** National Bureau of Standards

For a practical application, the acceleration field Γ can be represented by the two vector components: Γ_3 parallel to the y' axis (therefore perpendicular to the plane of the crystal), and Γ_1 in the crystal plane,

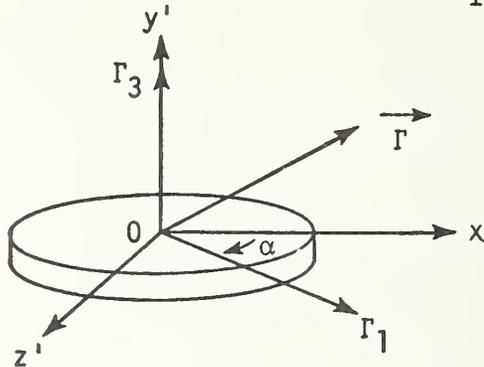


FIGURE 2 Decomposition of the generalized vector, Γ , into two components, Γ_3 and Γ_1 , which are referenced to the x and y' crystallographic axis.

where α is the azimuth angle between Γ_1 and the X crystallographic axis. See Fig. 2.

Rotating the crystal plate around the y' axis, it is possible to find some particular values of α for which the sensitivity due to Γ_1 is approximately zero.

For a given crystal technology, the effect of Γ_3 cannot be reduced with only one crystal. However, using two crystal resonators oriented as mirror images with respect to the y' axis connected in series can lead to first-order cancellation of the acceleration effect.

Fig. 3 shows the equivalent circuit for two crystal resonators connected in series.

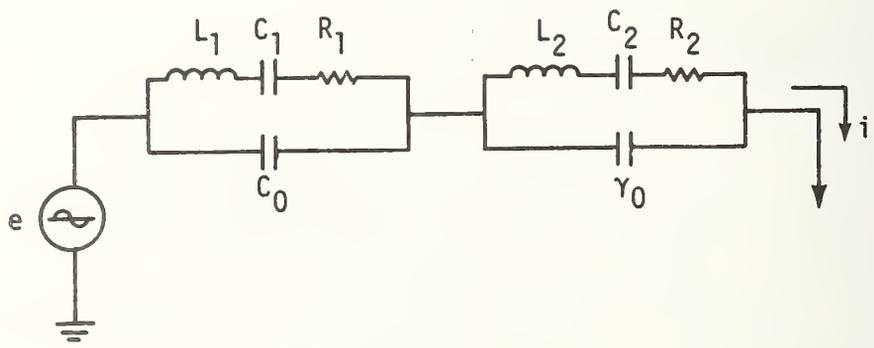


FIGURE 3 The equivalent circuit for two crystal resonators connected in series.

Solving the equation for $\left|\frac{i}{e}\right|^2$ yields:

$$\left|\frac{i}{e}\right|^2 = \frac{[uv - R_1 R_2 C_0 \gamma_0 \omega_1 \omega_2] + [R_1 C_0 \omega_1 v + R_2 \gamma_0 \omega_2 u]}{[R_1 v + R_2 u - 2L_1 \omega_1 R_2 \gamma_0 \omega_2 - 2L_2 \omega_2 R_1 C_0 \omega_1 y]^2 + [R_1 R_2 (C_0 \omega_1 + \gamma_0 \omega_2) + 2L_1 \omega_1 x v + 2L_2 \omega_2 y \omega]^2}$$

with $u = 1 - 2L_1 C_0 \omega_1^2$

$v = 1 - 2L_2 \gamma_0 \omega_2^2 y$

$x = \frac{\Delta f}{F_1}$ $y = \frac{\Delta f - \epsilon}{F_2}$ $\Delta f = F - F_1$ $4\pi^2 F_1^2 = \frac{1}{L_1 C_1}$

F is the driving frequency,
 F_1 is the series resonance frequency of the 1st resonator, F_2 is the series resonance frequency of the 2nd resonator and ϵ is the difference between the frequencies F_1 and F_2 .

Calculated variations of $\left|\frac{i}{e}\right|$ as a function of the driving frequency and various parameters are represented in Fig. 4,5,6, and 7:

- Fig. 4) Parameter: parallel capacitor C_0 ; $F_1 = 10$ MHz,
- Fig. 5) Parameter: λ_0 ; $F_1 = 10$ MHz,
- Fig. 6) Parameter: L_2 $F_1 = 10$ MHz,
- Fig. 7) Parameter: ϵ ; $F_1 = 10$ MHz.

Figure 8 shows the experimental results obtained with a pair of 3rd overtone AT cut 10 MHz crystals whose resonance frequencies are widely separated. Figure 9 shows the experimental results with a pair of 3rd overtone AT cut 10 MHz crystals. Figure 10 shows the results for a pair of 5th overtone AT cut 5 MHz crystals manufactured at the Ecole Nationale Supérieure de Chronometrie et Micromécanique (ENSCM).

The experimental curves verify that the series connected resonators essentially produce a single resonance curve even when the individual resonance frequencies differ by more than the linewidth. This means that

resonators need only be reasonably close in frequency which is easily satisfied by current manufacturing tolerances. In fact the separation of curves A and B in Fig. 8 (350 Hz is more than 5 times larger than standard tolerance for these types of crystals .

Using crystal blanks from Manufacturer A, two resonators have been mounted using glass tubes as supports, their individual resonance frequencies were:

Quartz A) $F_0 = 10\ 000\ 155\ \text{Hz},$

Quartz B) $F_0 = 9\ 998\ 805\ \text{Hz}.$

These resonators were connected in series and used in the circuit shown in Fig. 11. The frequency response has two peaks: a very small one at $F = 10\ 000\ 800\ \text{Hz}$ and a large one at $f = 9.999\ 049\ \text{Hz}$ which was used for the measurements.

This circuit was mounted on a loudspeaker and subjected to vibrations at a frequency of 500 Hz.

a) For constant amplitude sinusoidal acceleration in the Γ_3 or y' direction the phase variation amplitudes which is proportional to the frequency difference between the compound crystal resonator and the driving frequency, was:

Quartz A alone: amplitude 0.07 V per arbitrary unit of acceleration

Quartz B alone: amplitude 0.15 V

Quartz A + B: amplitude 0.05 V

b) By proper rotations of the crystals about the y' axis the acceleration sensitivity could be reduced to the noise level, or less than .01 div. The noise was primarily due to thermal transient effects caused by the lack of enclosures around the resonators.

Although the two individual resonators do not have the same acceleration sensitivities, the compound crystal nevertheless, exhibits a substantial reduction in acceleration sensitivity. Also the acceleration sensitivities of production crystals should be inherently much more closely matched than these two prototype crystals. It therefore appears that a factor of 10 reduction in acceleration sensitivity can be achieved without elaborate matching techniques.

These first experiments show qualitatively that it is possible to decrease the total acceleration sensitivity of a quartz crystal oscillator using two resonators in series. Further work in this area needs to be done to quantitatively demonstrate the amount of acceleration desensitization that can be achieved .

To obtain quantitative results, improved mounting including good enclosures and an improved measurement system are necessary.

Reference [1] Influence of environment conditions on a quartz resonator. M. Valdois, J.J. Gagnepain, J. Besson. Proc. 28th Annual Freq. Contr. Symp., Fort Monmouth, NJ, 1974.

Acknowledgment

We would like to thank S. Jarvis for writing the computer program used in calculating the effect of various parameters on the resonator behavior of the resonators.

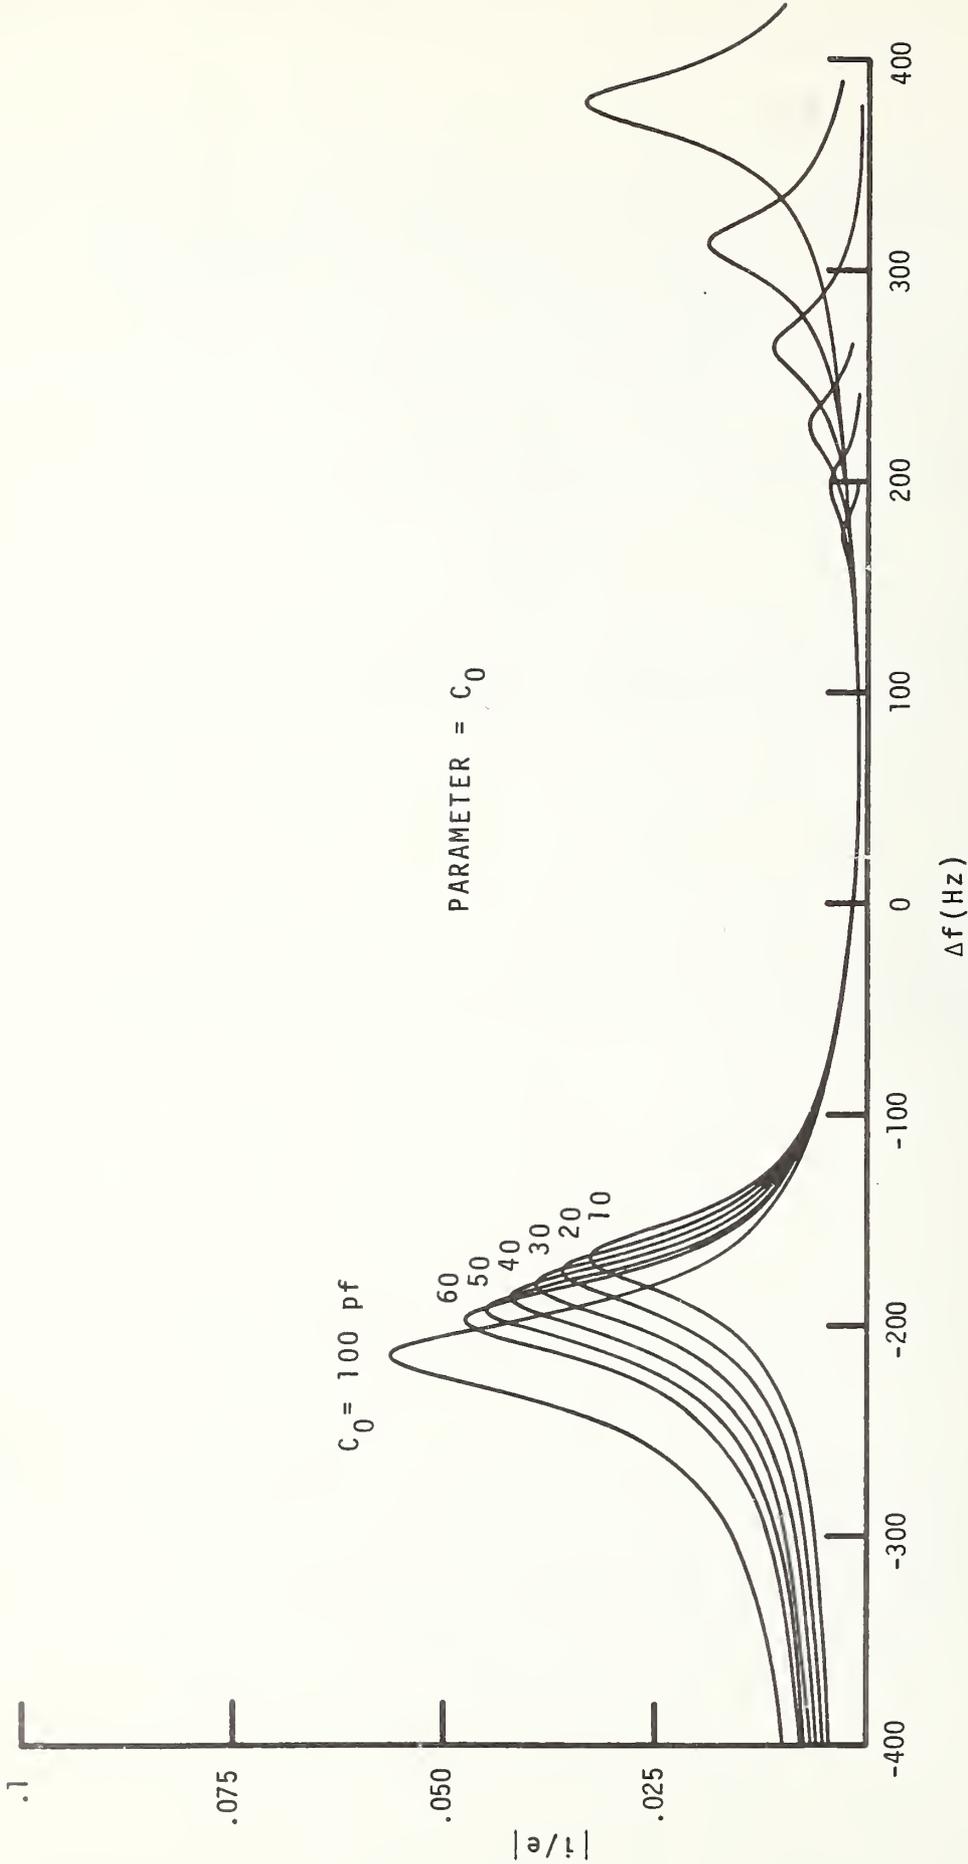


FIGURE 4 Calculated variation of $|1/e|$ as a function of Δf , the difference between the driving frequency and the resonator frequency of the first resonator and C_0 , the parallel capacitance across the first resonator. Other parameters were: $\epsilon = -300 \text{ Hz}$, $\gamma_0 = 50 \text{ pf}$, $L_1 = 0.1 \text{ H}$, $L_2 = 0.07 \text{ H}$, $R_1 = 15\Omega$, $R_2 = 17\Omega$, $F_1 = 10 \text{ MHz}$.

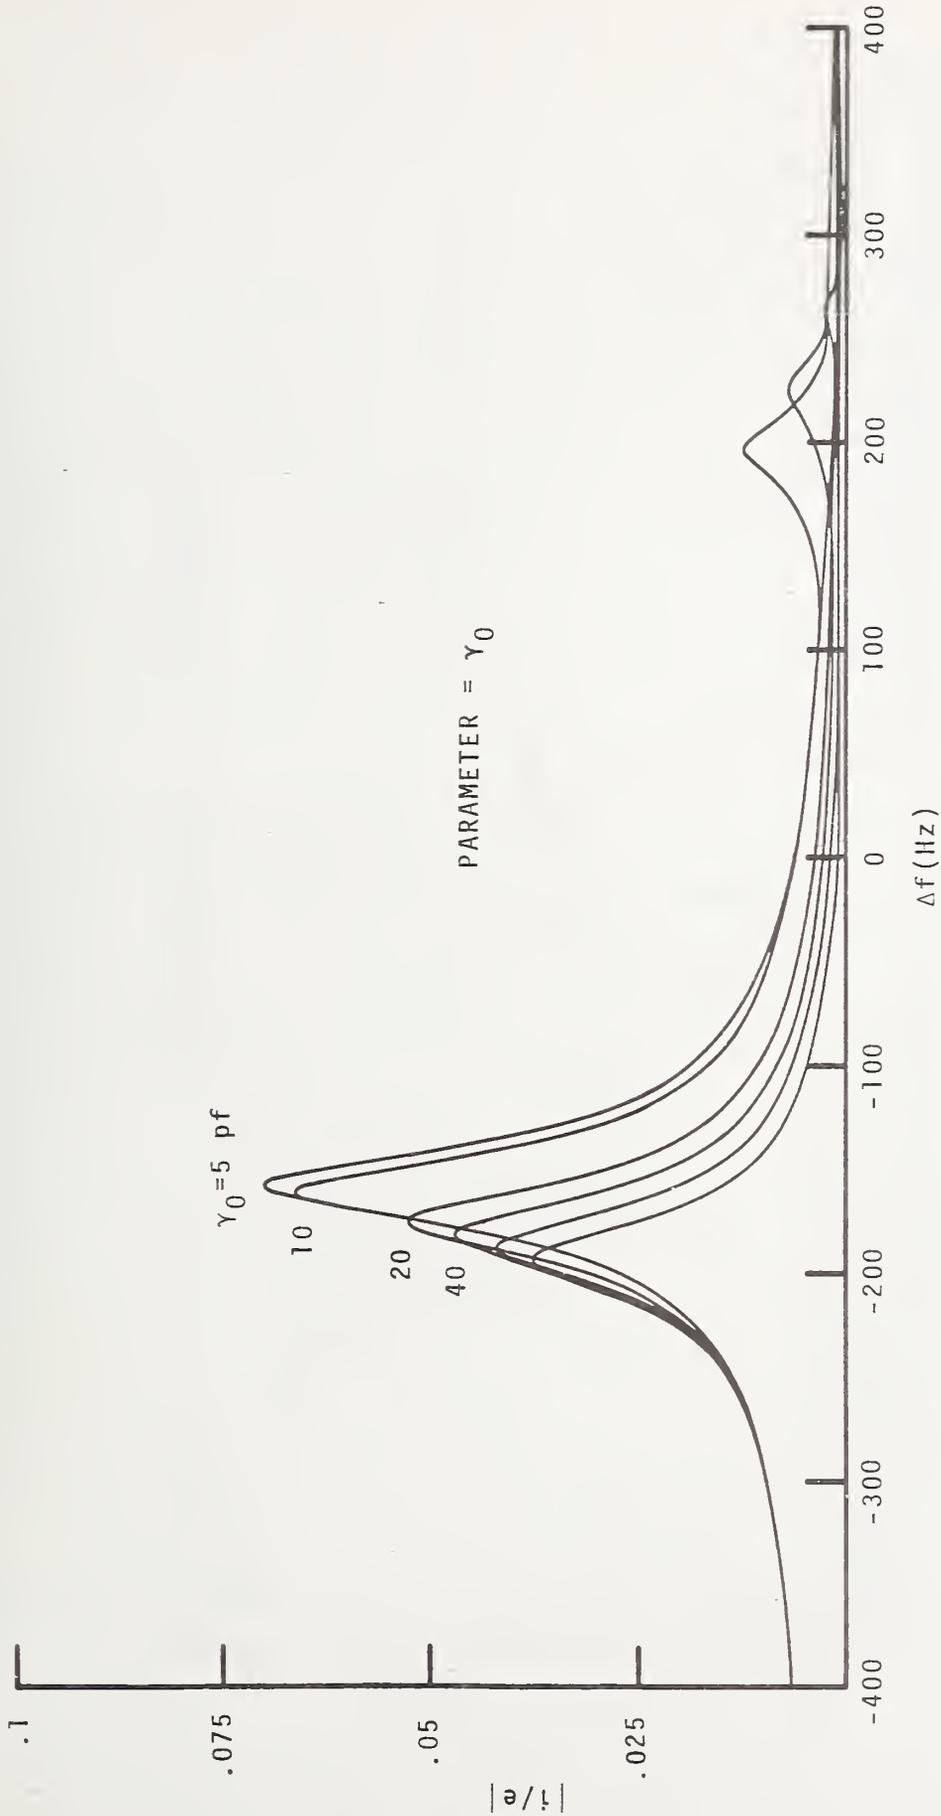


FIGURE 5 Calculated variation of $|1/e|$ as a function of Δf and γ_0 , the parallel capacitance across the second resonator. Other parameters were: $\epsilon = -300$ Hz, $C_0 = 40$ pf, $L_1 = 0.1$ H, $L_2 = 0.07$ H, $R_1 = 15\Omega$, $R_2 = 17\Omega$ and $F_1 = 10$ MHz.

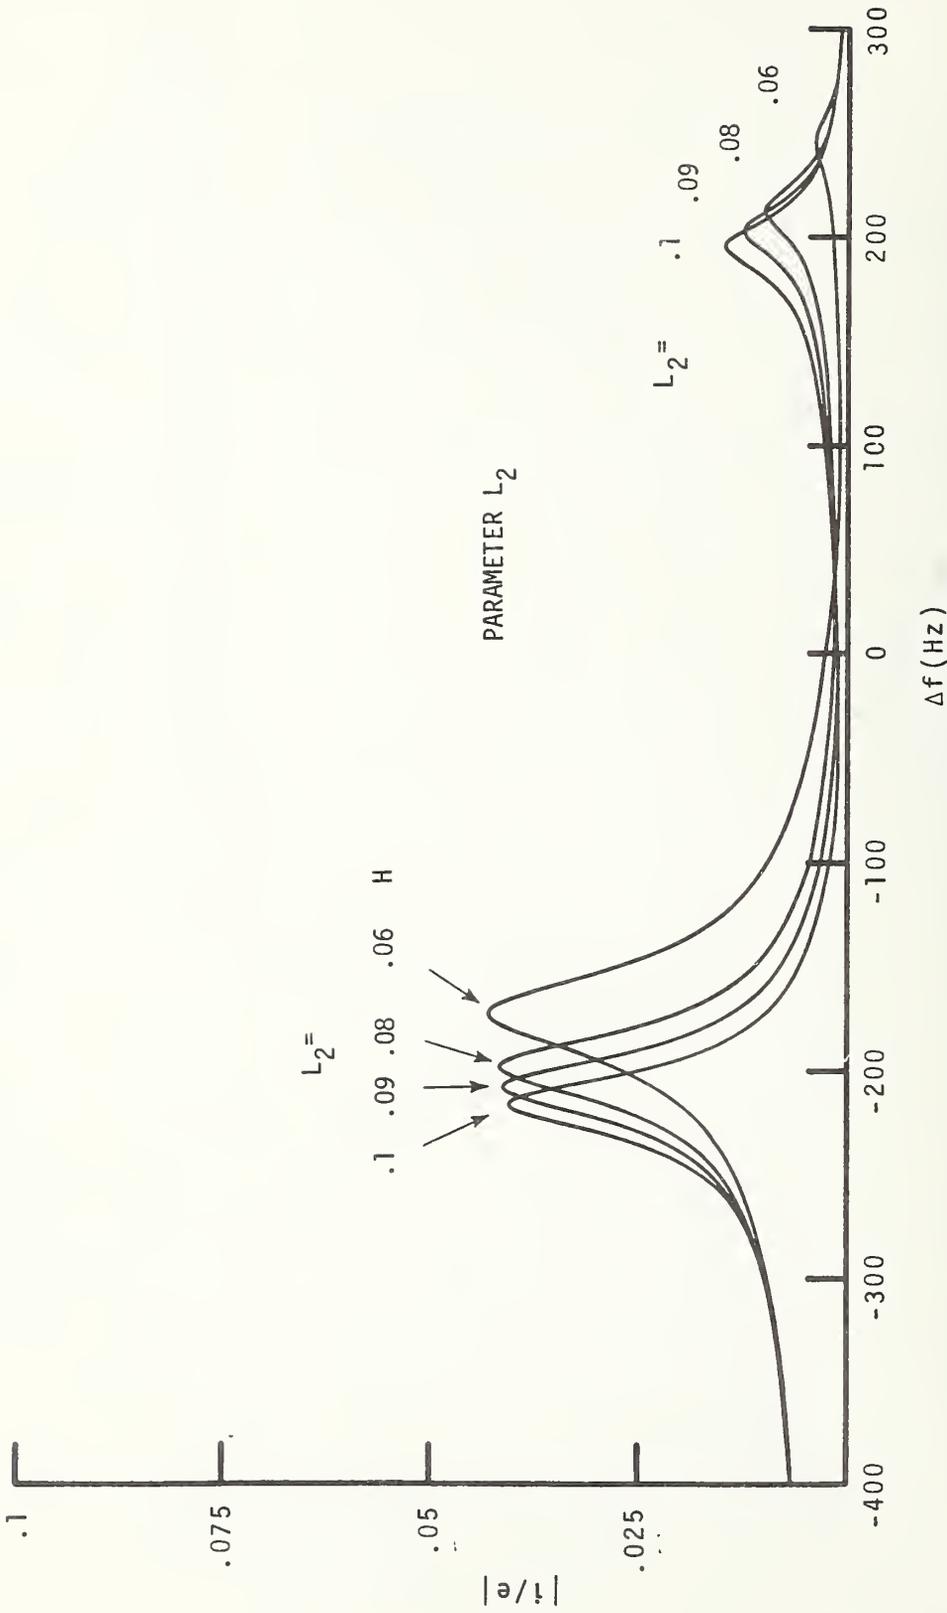


FIGURE 6 Calculated variation of $|i/e|$ as a function of Δf and ΔL_2 , the change in series inductance of the second resonator in H. Other parameters were: $\epsilon = -300$ Hz, $C_0 = 40$ pf, $\gamma_0 = 50$ pf, $L_1 = 0.1$ H, $R_1 = 15\Omega$, $R_2 = 17\Omega$, and $F_1 = 10$ MHz.

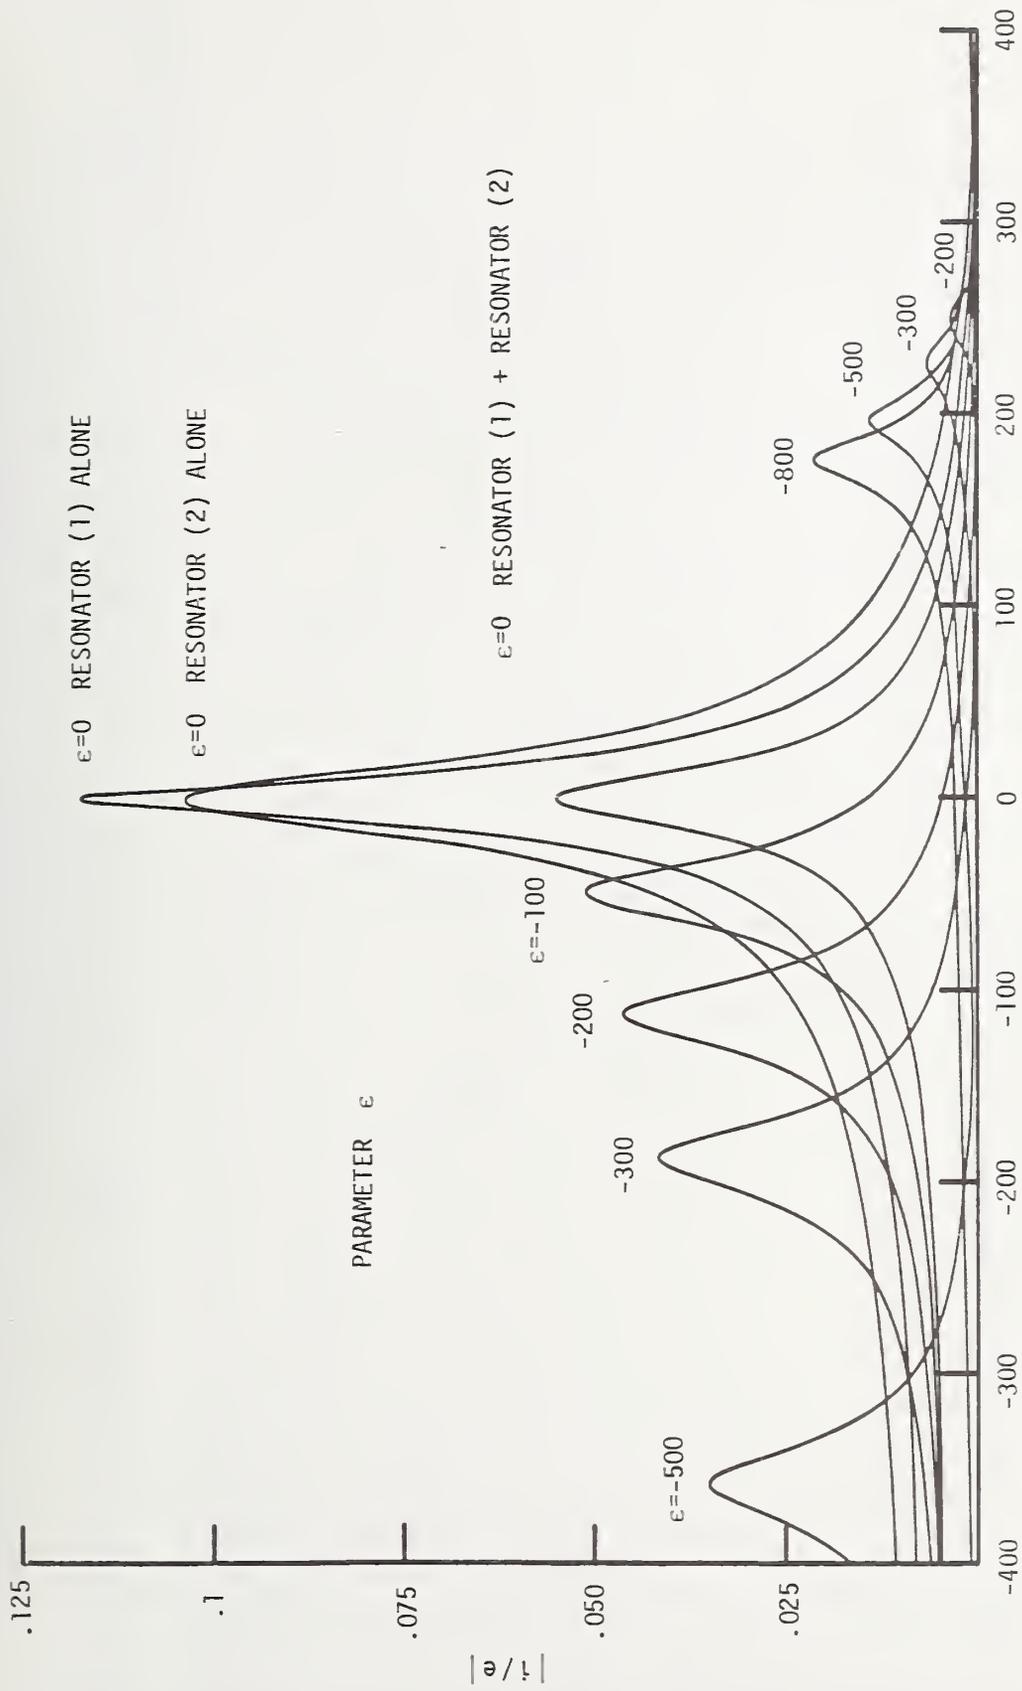


FIGURE 7 Calculated variation of $|1/e|$ as a function of Δf and ϵ , the frequency difference between the two resonators. Other parameters were: $C_0 = 40$ pf, $\gamma_0 = 50$ pf, $L_1 = 0.1$ H, $L_2 = 0.07$ H, $R_1 = 15\Omega$, $R_2 = 17\Omega$, and $F_1 = 10$ Hz.

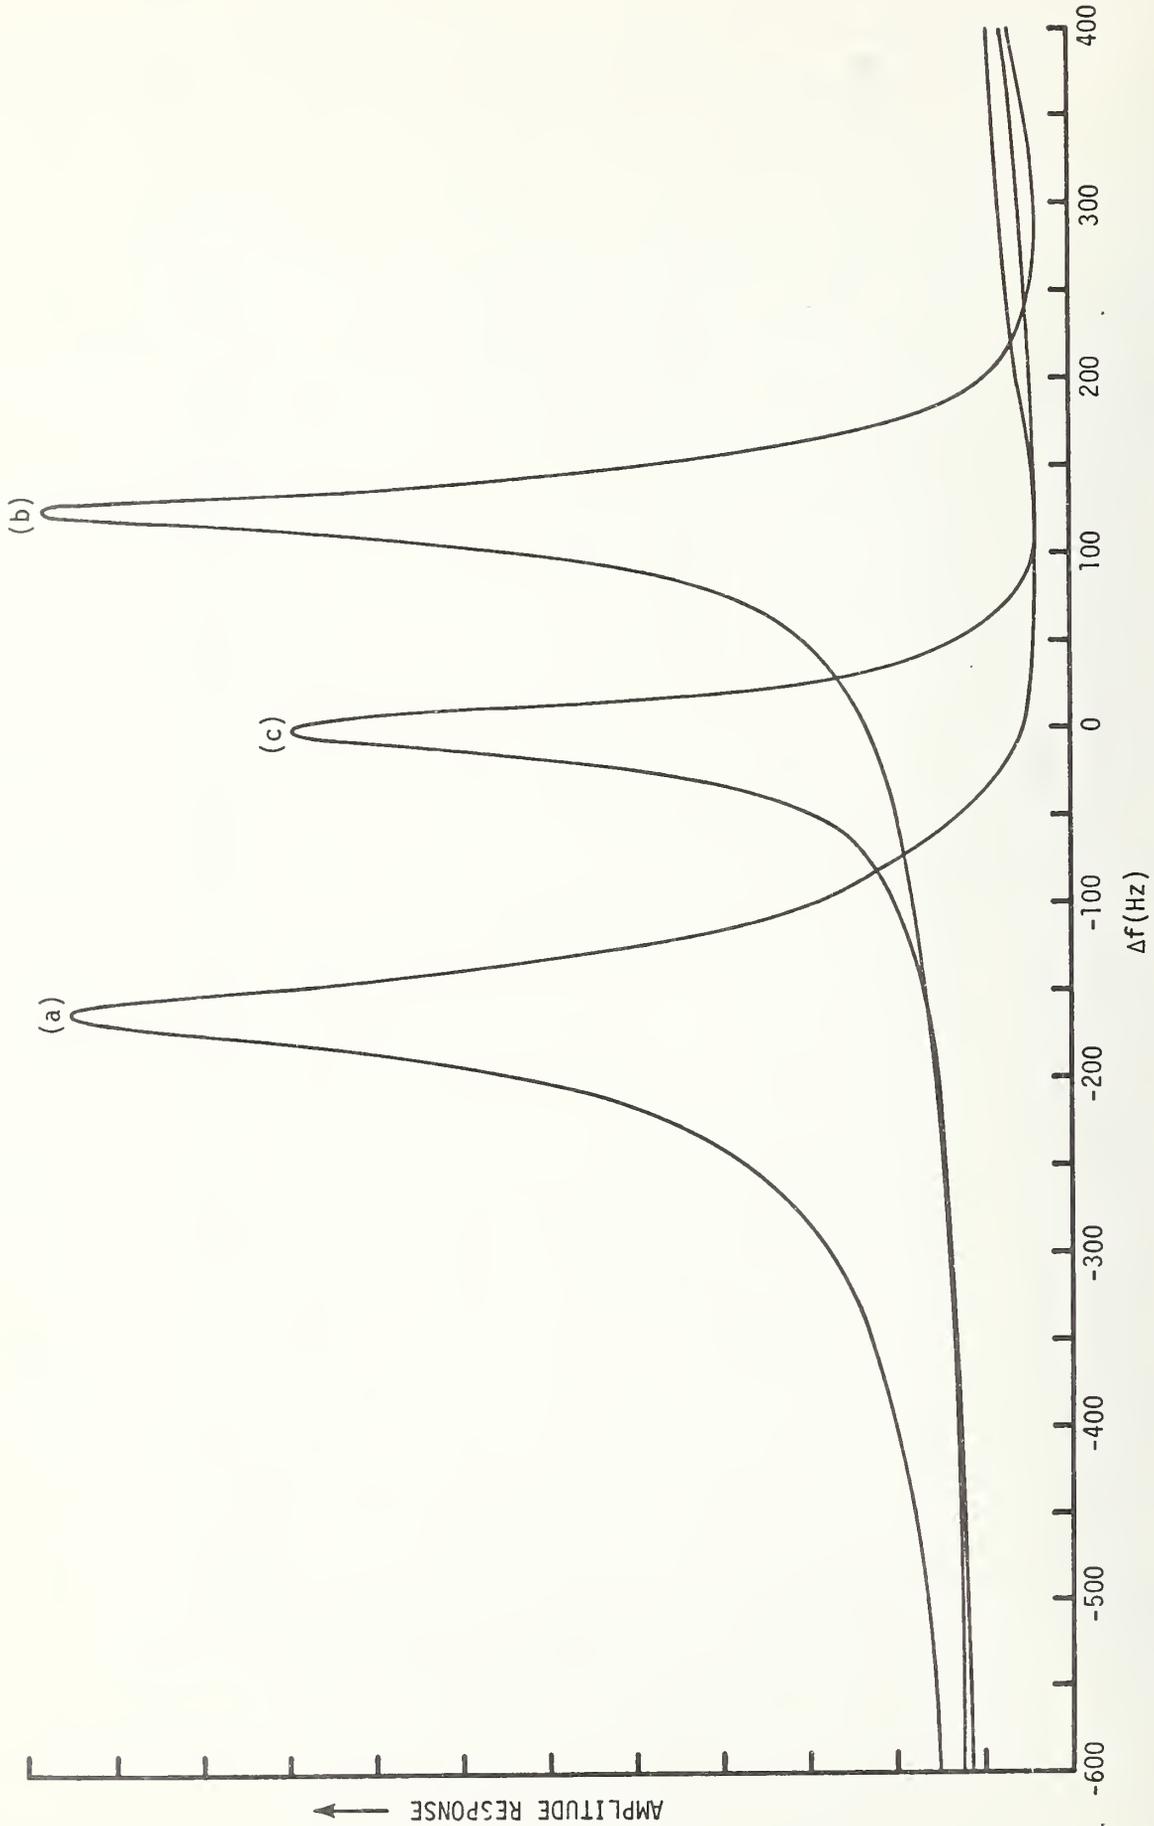


FIGURE 8 Experimental amplitude response as a function of driving frequency of: a) and b) single 3rd overtone crystals from Manufacturer A and c) the two crystals connected in series. Note the single resonance.

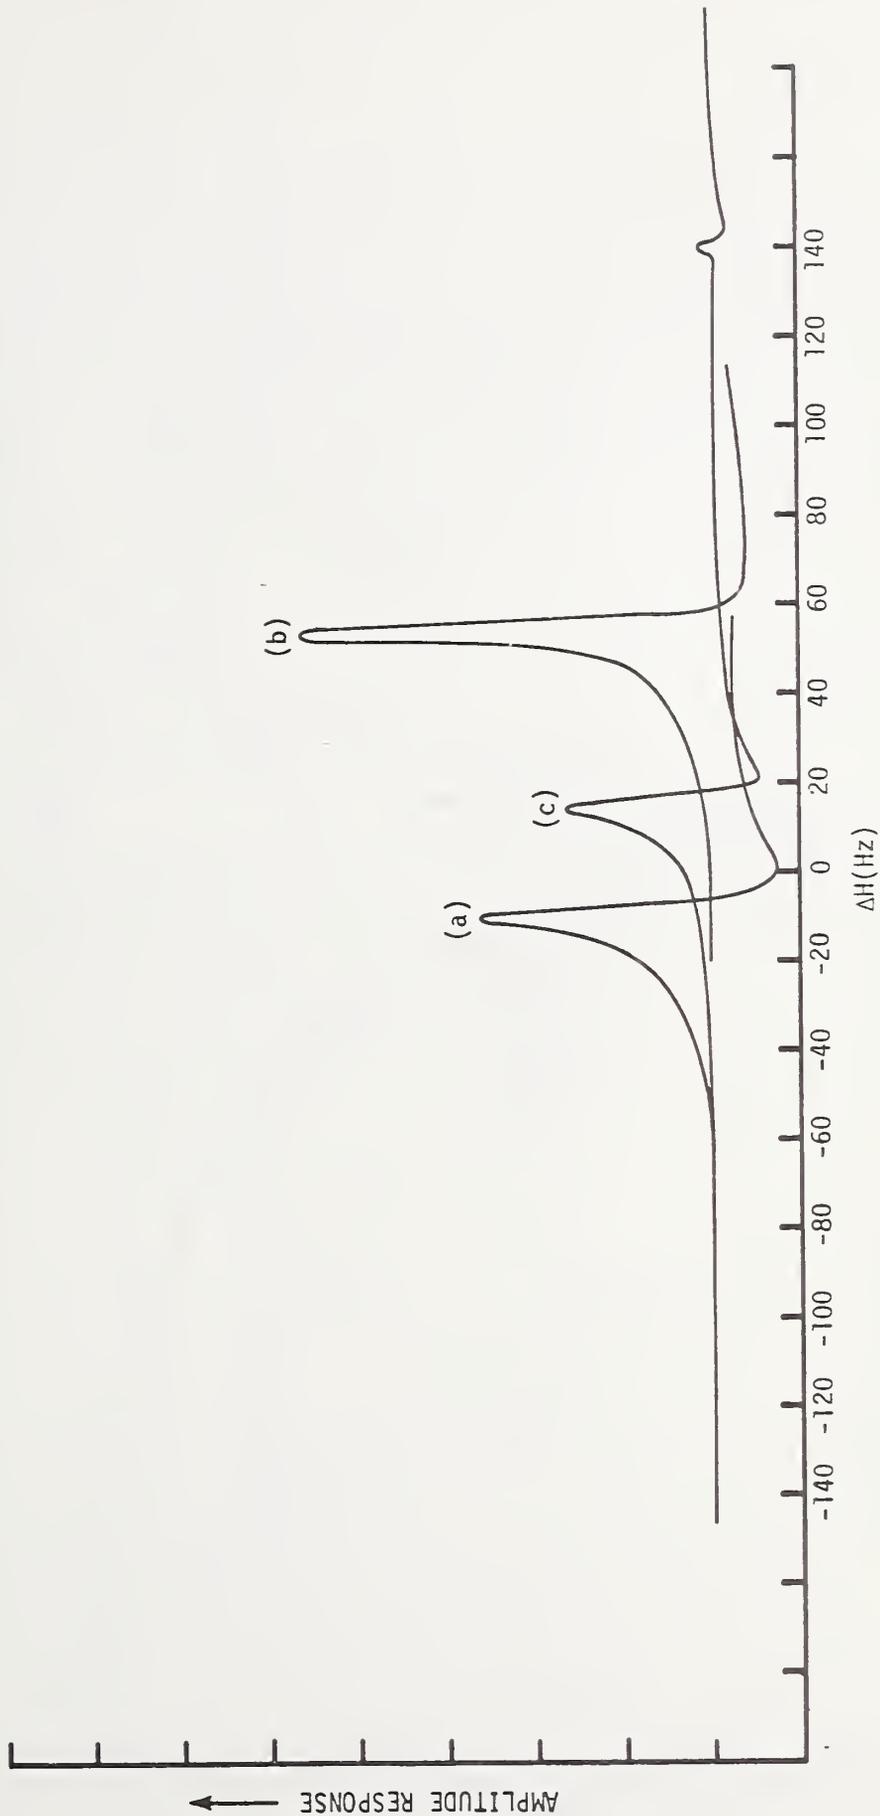


FIGURE 9 Experimental amplitude response as a function of driving frequency of a) and b) single 3rd overtone At cut 10 MHz crystals from Manufacturer B, and c) the two crystals connected in series. Note the single resonance.

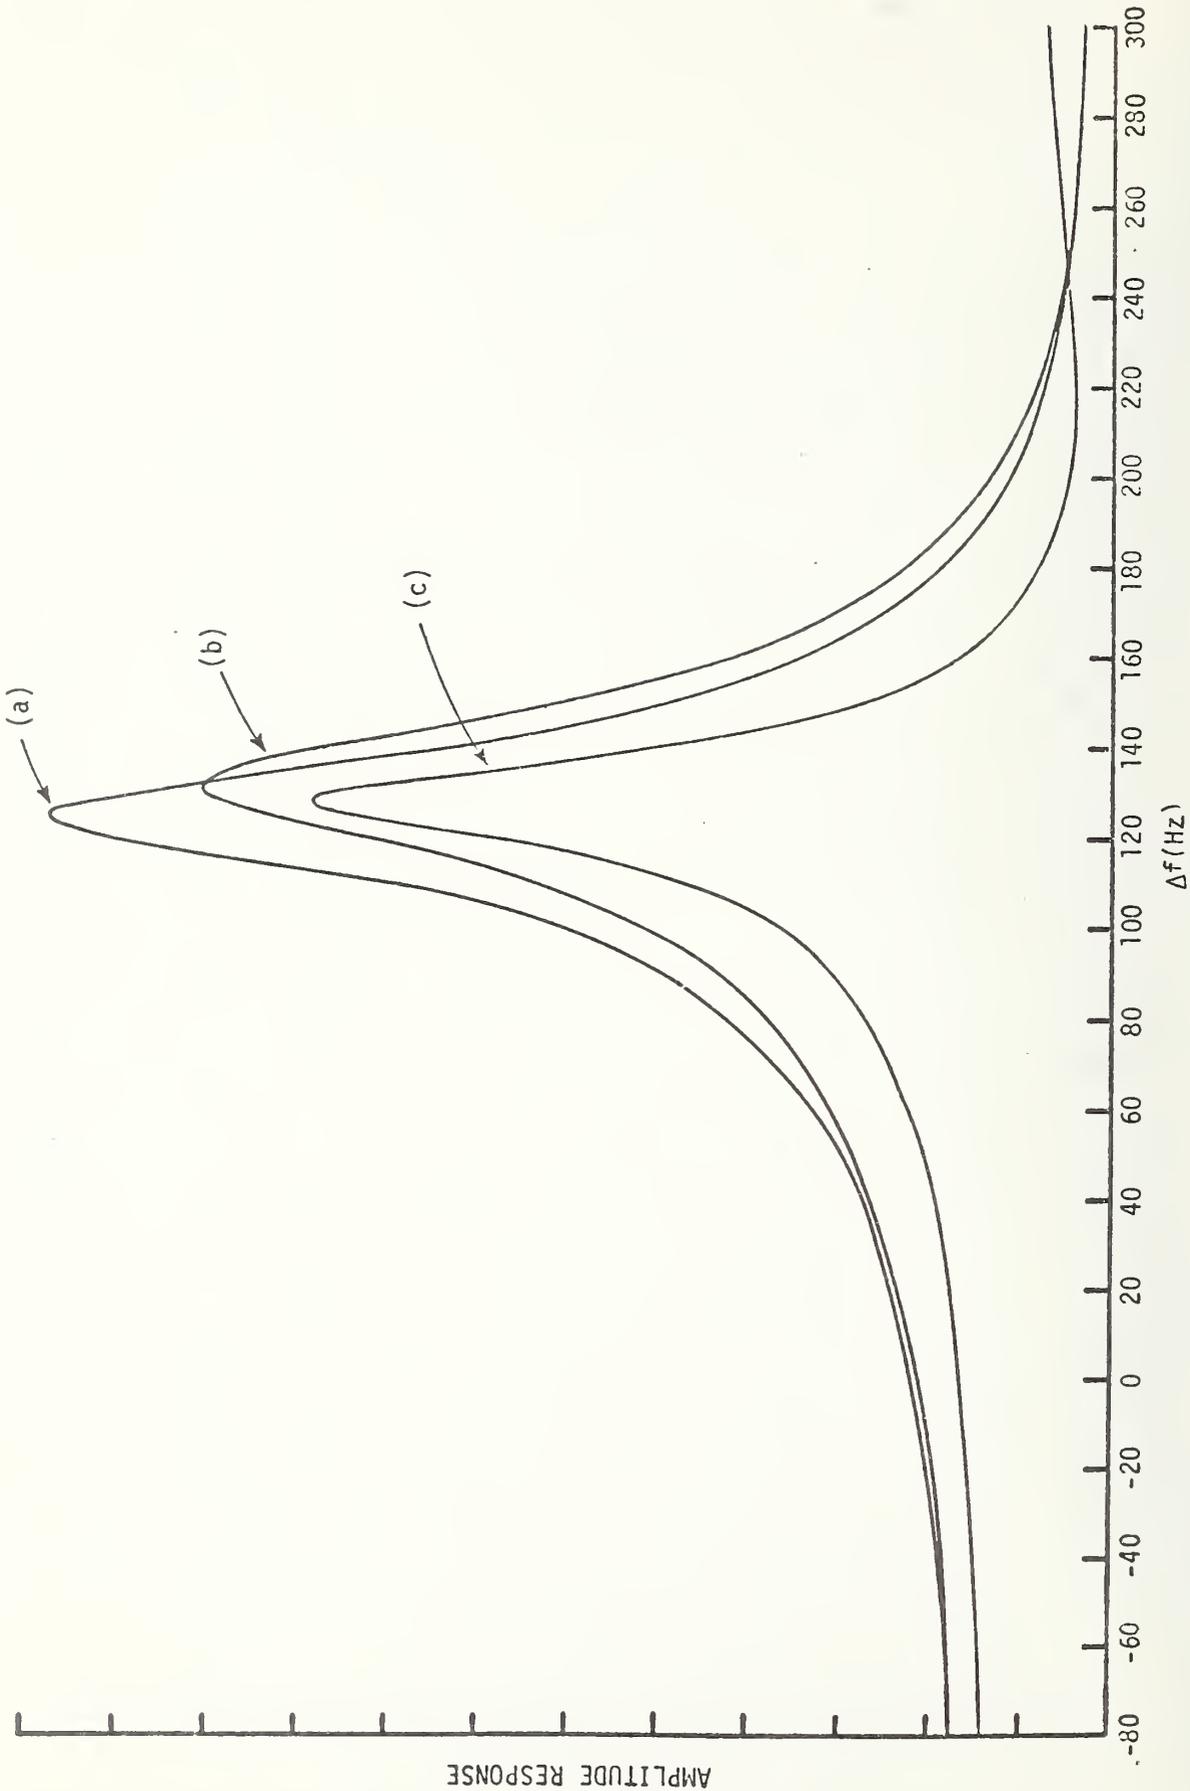


FIGURE 10 a) Amplitude response vs. driving frequency for:
 (a) a 5th overtone 5 MHz crystal #EN SCM 5061
 (b) a 5th overtone 5 MHz crystal #EN SCM 5071
 (c) the two crystals in series. Note the single resonance.

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET	1. PUBLICATION OR REPORT NO. NBSIR 77-855	2. Gov't Accession No.	3. Recipient's Accession No.	
4. TITLE AND SUBTITLE QUARTZ CRYSTAL OSCILLATORS WITH LOW ACCELERATION SENSITIVITY		5. Publication Date March 1977	6. Performing Organization Code 277.04	
7. AUTHOR(S) J. J. Gagnepain and F. L. Walls		8. Performing Organ. Report No.		
9. PERFORMING ORGANIZATION NAME AND ADDRESS NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, D.C. 20234		10. Project/Task/Work Unit No. 2774246	11. Contract/Grant No.	
12. Sponsoring Organization Name and Complete Address (Street, City, State, ZIP)		13. Type of Report & Period Covered	14. Sponsoring Agency Code	
15. SUPPLEMENTARY NOTES				
<p>16. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here.)</p> <p>The acceleration sensitivity of quartz crystal resonators imposes severe limitation on their use in non-laboratory environments. This work shows that by using two resonators connected in series and properly orientated with respect to one another, it is possible to substantially reduce the net acceleration sensitivity of the composite or compound crystal resonator. First qualitative experimental results on acceleration, also some experimental theories of studies related to the introduction of the two resonators comprising the compound resonator, are presented. From these studies it appears feasible to fabricate compound crystal resonators exhibiting acceleration sensitivities at least 10 times smaller than the resonators used individually.</p>				
<p>17. KEY WORDS (six to twelve entries; alphabetical order; capitalize only the first letter of the first key word unless a proper name; separated by semicolons)</p> <p>Acceleration field; acceleration sensitivity, compound crystal resonator; crystallographic axis; non-linear elastic effect; resonance frequency</p>				
<p>18. AVAILABILITY</p> <p><input checked="" type="checkbox"/> Unlimited</p> <p><input type="checkbox"/> For Official Distribution. Do Not Release to NTIS</p> <p><input type="checkbox"/> Order From Sup. of Doc., U.S. Government Printing Office Washington, D.C. 20402, SD Cat. No. C13</p> <p><input checked="" type="checkbox"/> Order From National Technical Information Service (NTIS) Springfield, Virginia 22151</p>	<p>19. SECURITY CLASS (THIS REPORT)</p> <p>UNCLASSIFIED</p>	<p>21. NO. OF PAGES</p> <p>15</p>	<p>20. SECURITY CLASS (THIS PAGE)</p> <p>UNCLASSIFIED</p>	<p>22. Price</p> <p>\$3.50</p>